


Software Version : 6.3.2.0646
Sample Name : ETHANOL FOR EVAL.
Instrument Name : Clarus 500 GC 1
Rack/Vial : 0/0
Sample Amount : 1.000000
Cycle : 1

Date : 10/30/2013 11:57:46 AM
Data Acquisition Time : 10/30/2013 11:31:28 AM
Channel : B
Operator : TC01GC
Dilution Factor : 1.000000

Result File : C:\TC Files\TC Data\2013\GC 1\October\October126B.rst
Sequence File : C:\TC Files\Meth-Seq-Rpt\GC1\2013\October.seq

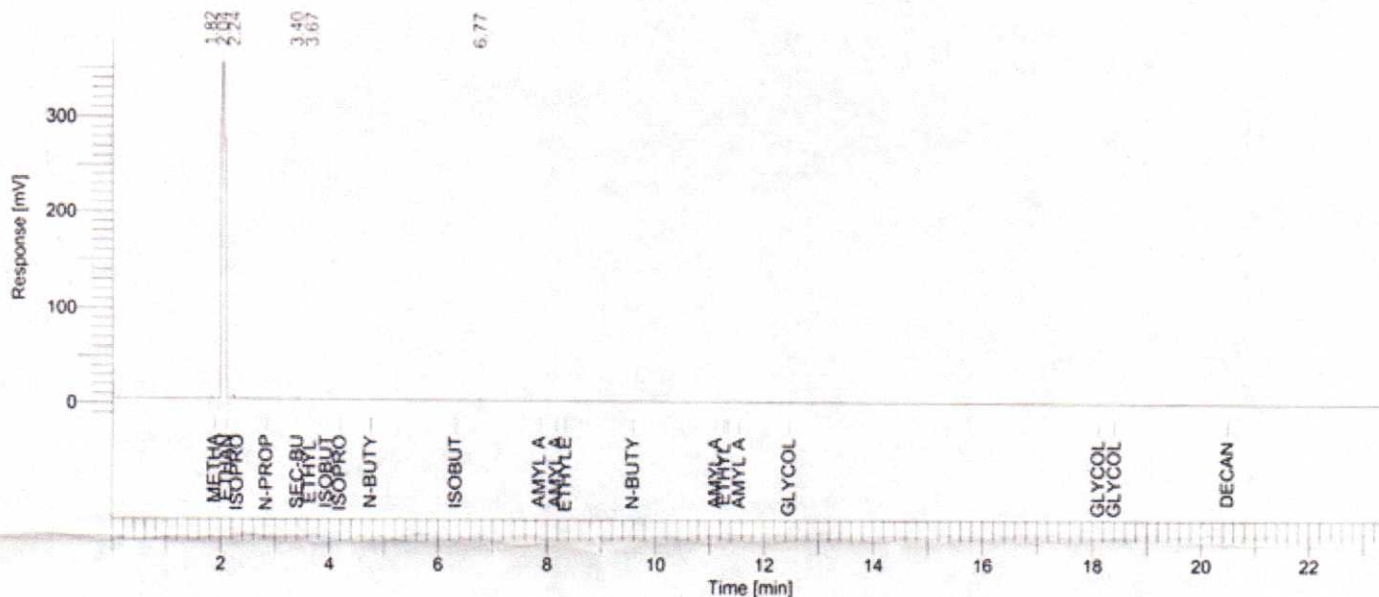

DEFAULT REPORT

Peak #	Time [min]	Area [μV-s]	Area [%]	BL	Component Name
1	1.82	3396.16	0.19	BB	
2	2.04	1803379.80	99.17	BB	
3	2.24	4273.21	0.23	BB	Isopropyl Alcohol
4	3.40	3094.32	0.17	BB	Sec-Butyl Alcohol
5	3.67	1132.92	0.06	BB	Ethyl Acetate
6	6.77	3182.46	0.18	BB	

1818458.85 100.00